

7 **Polymerization stress development in dental composites: Effect**
8 **of cavity design factor**

9 **Joseph M. Antonucci¹, Anthony A. Giuseppetti², Justin N.R. O'Donnell², Gary E. Schumacher²**
10 **and Drago Skrtic^{2*}**

11 ¹Polymers Division, National Institute of Standards and Technology, Gaithersburg, 20899, MD, USA

12 ²Paffenbarger Research Center, American Dental Association Foundation, Gaithersburg, 20899, MD,
13 USA

14 E-mails:

15 joe.antonucci@nist.gov; tony.giuseppetti@nist.gov; justin.odonnell@nist.gov; gary.schumacher@nist.gov;
16 drago.skrtic@nist.gov

17 * Author to whom correspondence should be addressed:

18 Drago Skrtic; Tel.: 301-975-3541; Fax: 301-963-9143

19

20 **Abstract:** The objective of the study was to assess the effect of the cavity design factor (C-
21 factor) on polymerization stress development (PSD) in resin composites. An experimental
22 resin (BT resin) was prepared, which contained 2,2-bis[p-(2'hydroxy-3'-
23 methacryloxypropoxy)phenylene]propane (B) and triethylene glycol dimethacrylate (T) in
24 1:1 mass ratio, and an activator for visible light polymerization. Also an experimental
25 composite with demonstrated remineralizing potential was formulated by inclusion into the
26 BT resin of zirconia-hybridized amorphous calcium phosphate (ACP) filler at a mass
27 fraction of 40 % (BT/ACP composite). A commercial glass-filled composite (TPH) was
28 used as a control. To assess the effect of the test geometry on PSD, C-factor was
29 systematically varied between 0.8 and 6.0 by varying the height of the cylindrical composite
30 specimens. The measured PSD values obtained by cantilever beam tensometry for
31 specimens with variable C-factors were normalized for mass to specimens with a C-factor of
32 1.33 (h=2.25 mm) as controls to give calculated PSD values. Degrees of vinyl conversions
33 (DC) attained in the TPH control and in the experimental BT/ACP composites were
34 measured by near-infrared spectroscopy. In both the TPH and BT/ACP composite series,
35 PSD_{calc} increased with the increasing C-factor, confirming the hypothesis that the C-factor
36 value influences PSD values. The higher PSD_{meas} and PSD_{calc} values for the experimental
37 BT/ACP composite compared to the commercial TPH composite probably reflect

1 differences in the type and mass of the resin and filler phases in the two types of composite.
2 These differences also account for the observed variation (21 %) in DC attained in a
3 BT/ACP composite 2 h after cure (69.5 %) and in the DC of the TPH composite (57.5 %)
4 having the same C-factor. The cavity design factor seems to play a key role in influencing
5 the PSD of bonded composites, but other factors such as composite mass and composition
6 also must be considered for their effects on PSD.

7 **Keywords:** amorphous calcium phosphate, cavity design factor, composite, resin,
8 polymerization stress, tensometry

9 1. Introduction

10 Since the introduction of dental composites into dentistry in the 1960's [1], considerable
11 developments in filler technology, resin and polymerization initiation systems, as well as
12 improvements in the adhesion of dental composites to tooth structure have significantly improved their
13 properties and expanded their clinical utility. However, in spite of improvements in bonding
14 properties, micro-leakage and gap formation, primarily at the dentin/composite interface, remain major
15 weaknesses of these materials [2]. The polymerization of methacrylate-based dental composites is
16 usually accompanied by significant shrinkage and the production of internal stresses that depend on
17 both material and processing variables [3, 4]. Despite many investigations, the highly complex
18 phenomenon of polymerization shrinkage development in polymeric dental restorative materials is not
19 fully understood and remains a significant clinical concern [5]. This phenomenon becomes even more
20 complex when the composite is bonded into cavities of variable configurations. During the photo-
21 polymerization of restorative composites, a complex network involving the resin and silanized filler
22 phases quickly forms at the gel point. The composite's elastic limit reaches a level that does not allow
23 enough relaxation to occur to compensate for the reduction in volume, and rapid buildup of stress
24 occurs both in the composite and at the composite/tooth interface. Any additional polymerization
25 shrinkage beyond the gel point adds to this internal stress that develops in the polymer matrix and its
26 interfaces with the filler particles. For composites bonded to enamel/dentin, polymerization shrinkage
27 is constrained and polymerization stress development (PSD) becomes more complex due to the
28 generation of interfacial stresses involving tooth structures, usually unevenly distributed along the
29 cavity walls and the bonded composite surface [6, 7].

30 A number of material as well as processing factors can contribute to PSD in composites. Filler
31 type and content, resin type and composition, and mode of polymerization determine the amount of
32 volumetric shrinkage, elastic modulus and PSD of the composite [8]. The polymerization process is
33 affected by the type and concentration of initiators, e.g. chemical vs. photochemical, which determine
34 reaction kinetics and degree of vinyl conversion (DC; [9]). PSD values also vary according to the ratio
35 of the bonded to the unbonded (free) surface area of the composite in a cavity, i.e., the configuration or
36 C-factor [10-12]. Although the PSD in photopolymerized dimethacrylate monomer systems has been
37 studied quite extensively [5, 6, 8, 9, 13-16], a fuller understanding of the kinetics of polymerization
38 shrinkage and the accompanying stress is still lacking. Similarly, how cavity configuration affects the
39 performance of bonded composite restoratives, adhesives and sealants [10-12, 17-19] also needs to be
40 better understood. Feilzer *et al.* [19] have hypothesized that a larger free surface area (lower C-factor

value) in the restorative composite would lead to lower PSD values by allowing greater plastic deformation to occur during polymerization before the gel point is reached.

The aim of this study was to test the above hypothesis by assessing by tensometry the effect of the cavity design factor (C-factor) on PSD in resin composites bonded to a silanized glass substrate as a model for composites bonded to surfaces of a dental cavity. Specifically, the objectives were to study how C-factor variations affect the PSD in a typical amorphous calcium phosphate (ACP)-based composite with demonstrated remineralizing potential [20-22] and a typical commercial glass-filled composite using a cantilever beam based tensometer [23].


2. Results and Discussion

PSD_{meas} and PSD_{calc} data obtained for the BT/ACP and TPH composite specimens for a range of cavity configuration factors (C-factors) between 0.8 and 6.0 (composite height from 3.75 mm to 0.50 mm) are given in **Table 1**. The PSD_{meas} varied between 5.80 MPa and 6.96 MPa in the BT/ACP composite series and between 2.78 MPa and 3.37 MPa in the TPH composites. For any given C-factor, the value of PSD_{meas} in BT/ACP composites more than doubled the value obtained in the corresponding TPH control. Also, data scattering was significantly lower for the TPH compared to BT/ACP composite specimens (SD values ranging from 0.05 MPa to 0.19 MPa vs. 0.06 MPa to 0.68 MPa). Plotting PSD_{meas} values obtained either for BT/ACP or for the TPH composite specimens as a function of composite specimen height showed practically no correlation between the two (**Figure 1**).

Table 1. Measured PSD (mean value \pm SD of three repetitive measurements) and the corresponding calculated PSD for BT/ACP and TPH composites as a function of C-factor.

C-factor	Composite height (mm)	BT/ACP composite PSD (MPa)		TPH composite PSD (MPa)	
		measured	calculated	measured	calculated
0.80	3.75	nd		2.78 \pm 0.07	1.67
0.86	3.50	5.80 \pm 0.55	4.39	2.91 \pm 0.05	1.87
1.00	3.00	6.21 \pm 0.27	4.66	2.70 \pm 0.07	2.03
1.33	2.25	6.55 \pm 0.19	6.55	3.16 \pm 0.19	3.16
2.50	1.20	6.79 \pm 0.34	12.73	3.37 \pm 0.08	6.32
3.00	1.00	6.96 \pm 0.06	14.73	nd	
6.00	0.50	6.83 \pm 0.68	26.09	2.82 \pm 0.17	12.69

Figure 1. PSD_{meas} as a function of specimen height. Indicated are the mean values ± one standard deviation (SD). Number of runs n= 3/experimental group..

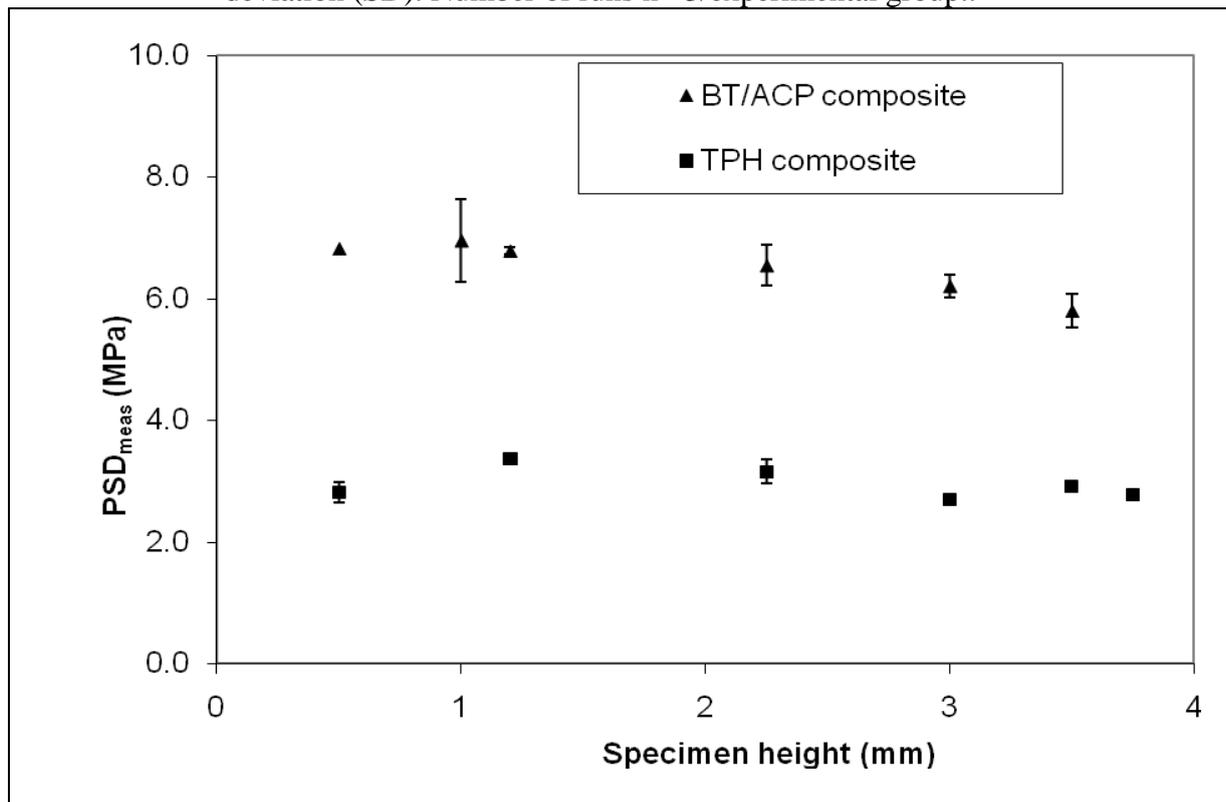

However, the corresponding PSD_{calc} values decreased with the increasing specimen thickness (height, h) for both the experimental and control groups (**Figure 2**) according to the following exponential functions (R^2 is the correlation coefficient):

$$\text{PSD(ACP)}_{\text{calc}} = 28.3 \cdot e^{-0.58h} \quad (R^2 = 0.9542) \quad (1)$$

$$\text{PSD(TPH)}_{\text{calc}} = 14.5 \cdot e^{-0.61h} \quad (R^2 = 0.9680) \quad (2)$$


Similarly, no correlation existed between the PSD_{meas} and C-factor for both types of composites (**Figure 3**). On the other hand, PSD_{calc} and the C-factor for both the BT/ACP and TPH composites (**Figure 4**) showed linear correlations that can be described by the following equations, respectively:

$$\text{PSD(ACP)}_{\text{calc}} = 4.28 \cdot \text{C-factor} + 1.05 \quad (R^2 = 0.9923) \quad (3)$$

$$\text{PSD(TPH)}_{\text{calc}} = 2.13 \cdot \text{C-factor} + 0.20 \quad (R^2 = 0.9903) \quad (4)$$


DC values attained in the BT/ACP and TPH composites at 1 min and 2 h after light-cure, shown in **Figure 5**, clearly indicate higher (21 % to 23 %) vinyl conversion in the BT/ACP composites compared to TPH control.

1 **Figure 2.** Functional dependence of PSD_{calc} (mean value \pm SD) on the specimen height. The
2 average PSD_{calc} values calculated from the mean PSD_{meas} data ($n = 3/group$).

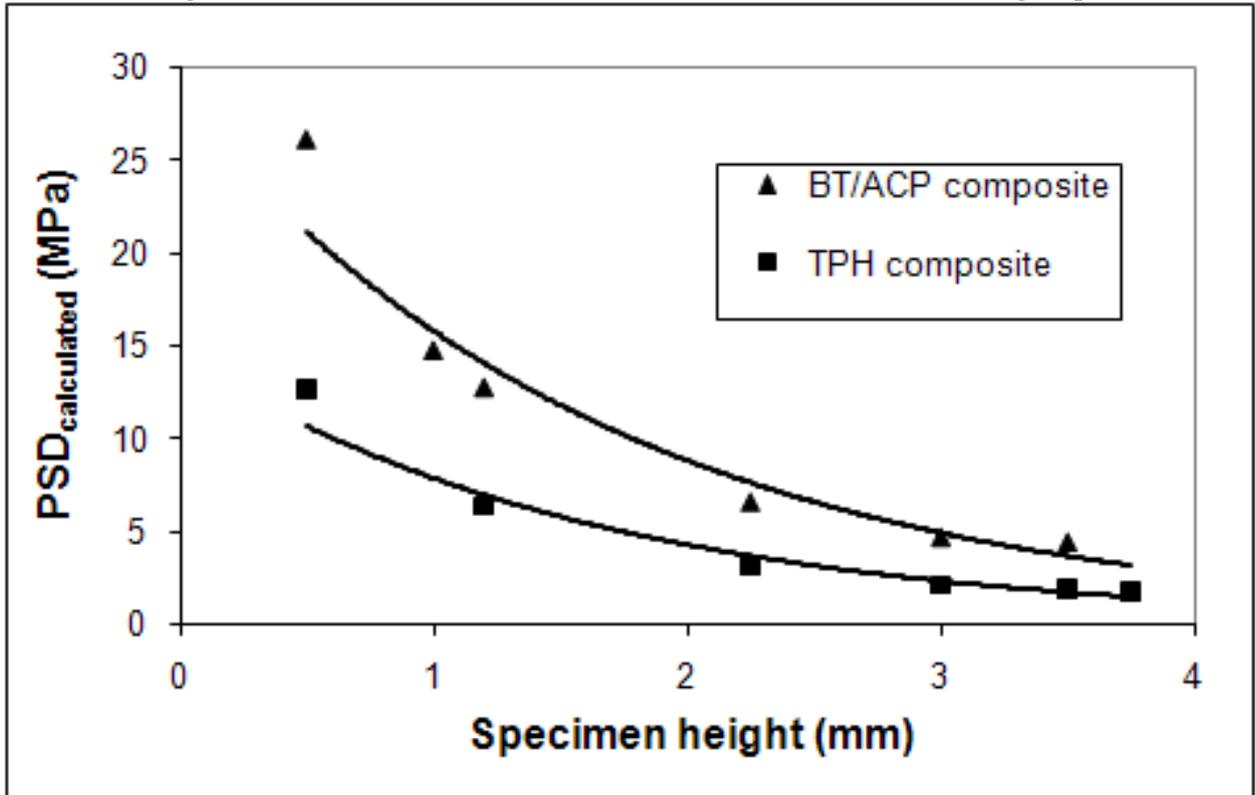


3
4
5

Figure 3. PSD_{meas} (mean value \pm SD) as a function of specimen height.

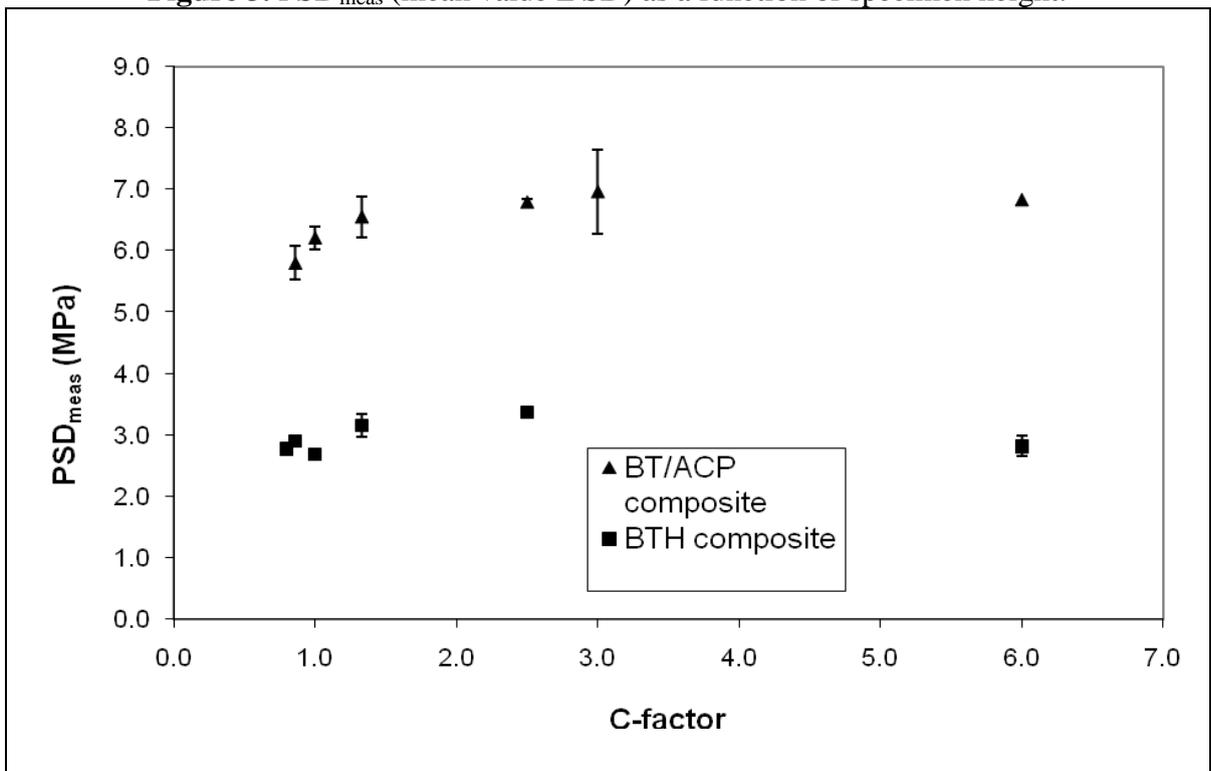


6
7
8

1 **Figure 4.** Functional dependence of PSD_{calc} on the cavity configuration factor. The average PSD_{calc}
 2 values calculated from the mean PSD_{meas} data ($n = 3/group$).

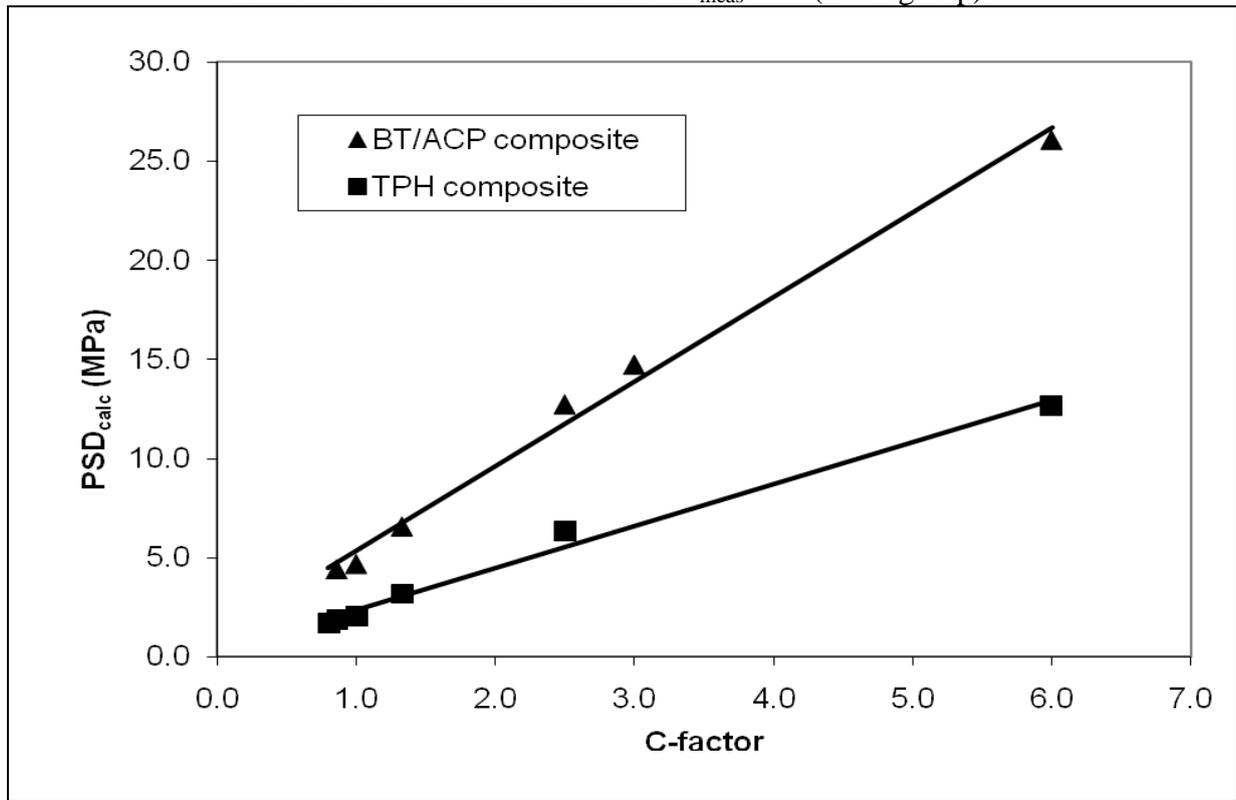

3
 4
 5 **Figure 5.** Degree of conversion (DC) attained 1 min and 2 h after visible light-curing of the
 6 BT/ACP and TPH composites, with the mean values of three repetitive measurements in each group;
 7 SDs are indicated.

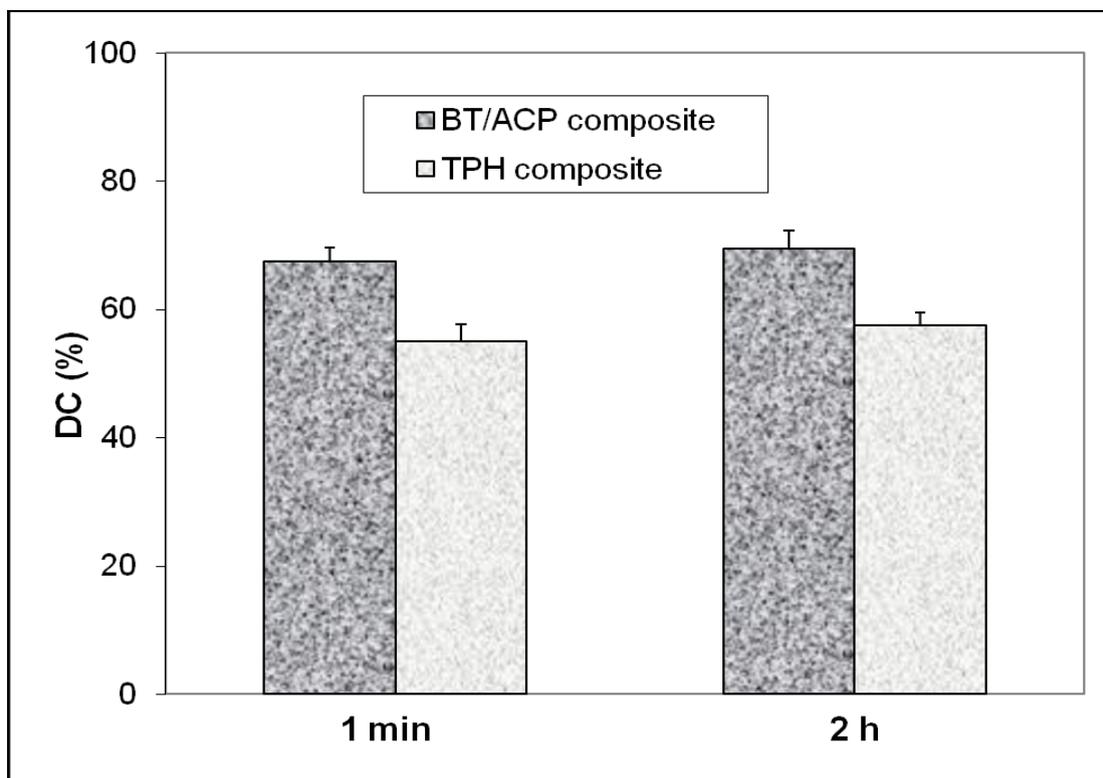

1 In this study an attempt was made to mimic the constrained polymerization shrinkage and stress
2 development that occurs in composites bonded to tooth structure. The silanized quartz surfaces mimic
3 bonding to flat dental surfaces via the use of dental adhesives also designed to chemically bond to
4 composite restoratives or inlays. Studies of PSD as a function of specimen thickness in applications
5 simulating the cementation of inlays, i.e. very thin layer of adhesive or composite [24, 25], have shown
6 a substantial disparity in stress with specimen height. For the range of specimen thickness examined in
7 our study (0.5 mm to 3.75 mm) no correlation was found between the PSD_{meas} and the specimen
8 thickness for both types of composites examined. One may attribute such findings to the lack of
9 instrument sensitivity to detect differences in PSD for composite specimens over the range of C-factors
10 studied. Watts and Satterthwaite [26] have, however, indicated that at specimen thicknesses more akin
11 to the resin-composite direct restorations, i.e., at thicknesses between 0.8 mm and 1.5 mm, the
12 variations in PSD tend to be minimal and are less affected by the instrument compliance. They have
13 shown that the uniaxial shrinkage stress/mass increases linearly with the increasing C-factor
14 (decreasing height of a specimen). Similar findings were reported by Lee et al. [27]. In this study
15 (**Table 1; Figure 4**) PSD_{calc} was directly proportional to C-factor confirming the original hypothesis.
16 However, PSD_{meas} data showed no correlation with either specimen thickness (height, h ; **Figure 1**) or
17 C-factor (**Figure 3**). The apparent discrepancy between the two data sets (PSD_{meas} vs. PSD_{calc}) remains
18 unexplained. Eq. (2) implies a simple relation between C-factor and 'h' that should be reflected in
19 PSD_{meas} .

20 Consistently higher PSD values for the experimental BT/ACP composite compared to the
21 TPH control composite reported in this study are not unexpected; the higher DC attained in the ACP
22 composite coupled with a significantly lower filler content would be expected to lead to higher
23 shrinkage upon polymerization and more stress development compared to the less converted and more
24 highly filled TPH composites. Not only the mass but also the type of filler used (a mass fraction of 40
25 % ACP without surface treatment in BT/ACP composites vs. a mass fraction of 78 % silanized glass
26 filler in TPH composite) can affect PSD. Also the greater translucency of the ACP composite
27 compared to TPH may enhance the degree of radiance of the former and contribute to the observed
28 higher DC. Another critical factor is the composition of the resin phase (Bis-GMA/TEGDMA
29 (BT/ACP composite) vs UDMA-modified Bis-GMA in TEGDMA (TPH composite)). Generally, the
30 urethane-modified Bis-GMA oligomer would be expected to shrink less than Bis-GMA/TEGDMA.
31 With respect to the PSD, it is generally beneficial to have high levels of fillers in composites since
32 their contribution, even when treated with coupling agents (e.g. silanized), to polymerization shrinkage
33 is minimal [28] but may contribute to PSD by increasing the elastic modulus. The filler content of the
34 resin-based composites has indeed been indicated as a major determining factor for PSD [10]. On the
35 other hand, the internal interfacial stress during the setting contraction of a resin composite is
36 proportional to elastic modulus (Young's modulus) of the material [29]. Other material factors being
37 equal, the most rigid material, i.e., the one with highest modulus will show the highest PSD with the
38 progression of polymerization reaction [30]. In view of the lack of correlation that existed between the
39 PSD_{meas} and C-factor for the composites, it could be informative to develop means to plot and
40 correlate the temperatures of the composites' exothermic polymerization, and the cooling that follows,
41 along with the measurement of the PSD [3].

42

1 3. Experimental Section

2 Resin formulation, ACP filler synthesis and characterization, composite preparation. The experimental
 3 resin was formulated from commercially available 2,2-bis[p-(2'hydroxy-3'-
 4 methacryloxypropoxy)phenylene]propane (Bis-GMA) and triethylene glycol dimethacrylate
 5 (TEGDMA) monomers in a 1:1 mass ratio (designated BT resin). Bis-GMA and TEGDMA were used
 6 as received from the manufacturer (Esstech, Essington, PA, USA) without additional purification. BT
 7 resin was photo-activated by the inclusion of a mass fraction 0.2 % camphorquinone and a mass
 8 fraction 0.8 % ethyl-4-N, N-dimethylamino benzoate.

9 The ACP remineralizing composite (designated BT/ACP composite) was formulated with a
 10 zirconia-hybridized amorphous calcium phosphate (Zr-ACP) filler (median particle diameter $d_m = (5.7$
 11 $\pm 2.2)$ μm). Composite paste was prepared by hand spatulation by combining mass fractions of 40 %
 12 Zr-ACP and 60 % BT resin. Zr-ACP was synthesized and characterized as detailed earlier [20]. The
 13 volume filler fraction of the experimental material is 30 %. Its shade is B1 compared to the VITAPAN
 14 Lumin Vacuum shade guide (Vita Zahnfabrik, Bad Säckingen, Germany). The observed slightly higher
 15 translucency is attributed to the relatively low filler content by volume. A commercial composite
 16 (TPH³ Micro Matrix Restorative: lot #070403, shade A1, Dentsply-Caulk, Milford, DE, USA) was
 17 used as control in this investigation. TPH³ consists of a visible-light activated, urethane-modified Bis-
 18 GMA, ethoxylated-Bis-GMA and TEGDMA (1:1:1 mass ratio). The composites contains mainly a
 19 barium boron aluminum silicate glass at a 78 % mass fraction level (filler volume fraction is approx.
 20 57 %).


21 Polymerization stress development (PSD) measurements. PSD was quantified by utilizing a computer-
 22 interfaced, cantilever beam tensometer developed at Paffenbarger Research Center, ADAF, at NIST,
 23 Gaithersburg, MD, USA (**Figures 6 and 7**). For a rectangular prismatic cantilever beam of a linearly
 24 elastic material with a small deflection, which is under a concentrated normal load F, the displacement
 25 at the end of the cantilever beam is defined by the following expression:

$$26 \quad \varepsilon/F = 2a^2(3L-a)/Ebd^3 \quad (5)$$

27 In equation (1), ε is the displacement at the beam end (μm); E is the Young's modulus of the cantilever
 28 beam (MPa); F is the load (N) needed to generate the displacement ε ; L is the total beam length (cm); a
 29 is the distance from the load-applied position to the end of the beam (cm); b is the width of the beam
 30 (cm) and d is the height of the beam (cm). The deflection of the cantilever beam was measured with a
 31 linear variable differential transformer. The force was calculated from a beam length (12.5 cm) and a
 32 calibration constant (3.9 N/ μm). PSD was obtained by dividing the measured force by the cross
 33 sectional area of the sample (diameter = 6 mm).

34

35 **Figure 6.** Schematic of a tensometer such as the one utilized in the study. In the present study,
 36 Tygon sleeves (instead of PTFE) encased the samples, and their inner surfaces represented the
 37 unbonded areas.
 38

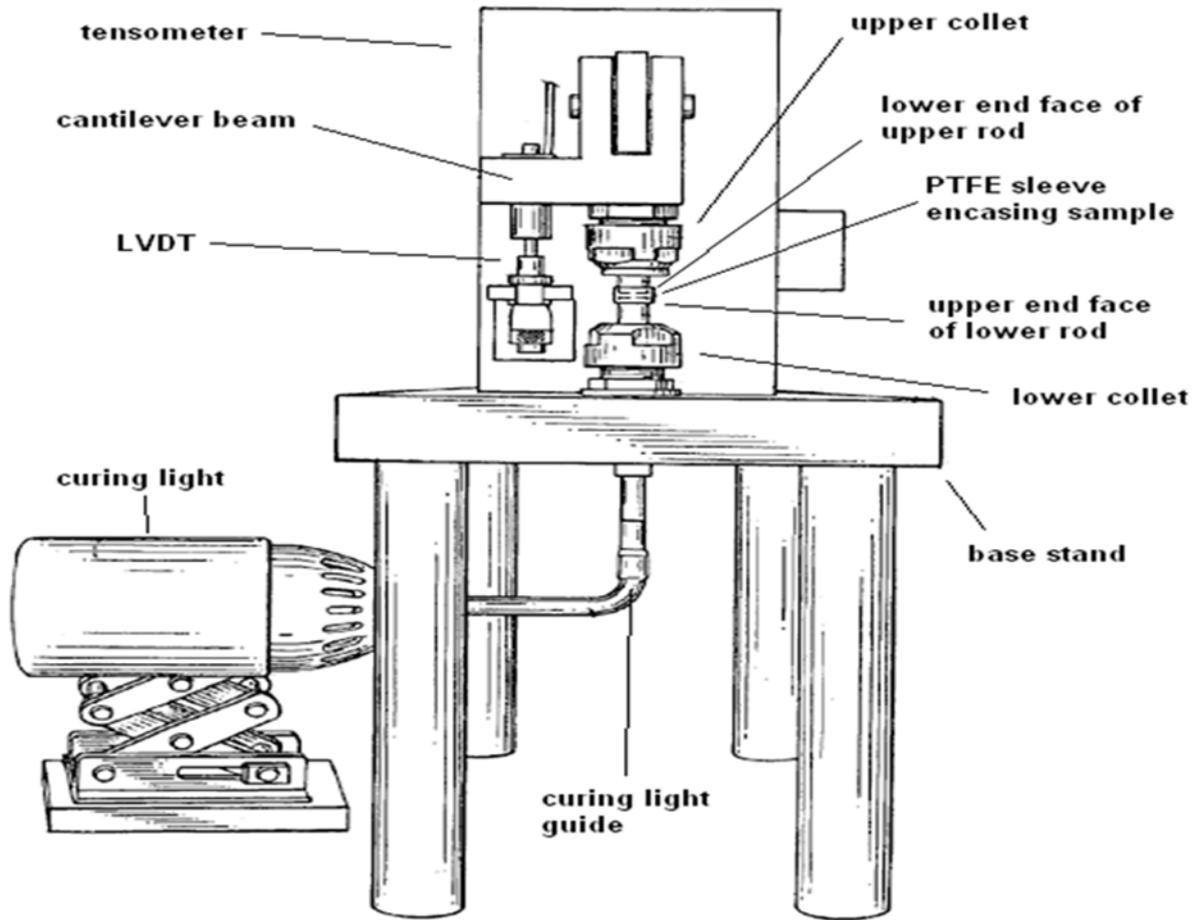

1
2
3
4
5
6

Figure 7. Positioning tygon (a), filling the mold (b) and light curing of the specimen (c) in the tensometer.



7
8



b



c

To systematically evaluate effects of different configurations on PSD, the heights (h) of unpolymerized composite cylindrical specimens were varied between 0.5 mm and 3.75 mm to give C-factors ranging from 6.0 to 0.8. For a circular quartz rod of diameter $2r$ and a specimen of height h , C-factor was calculated as the ratio of bonded composite area (the silanated ends of the silica rods) to the unbonded area (the compliant plastic enclosure) according to the expression:

$$\text{C-factor} = \frac{2\pi r^2}{2\pi r h} = r/h \quad (6)$$

The composites were irradiated through the lower quartz rod with a visible light (Spectrum Curing Unit, Dentsply-Caulk, Milford, DE, PA, USA) for 60 s to initiate polymerization, and the PSD was then measured after 60 min. The light intensity, measured by a Demetron Model 100 radiometer (Demetron Research, Danbury, CT, USA) was (510 ± 25) mW/cm² at the upper end of the top quartz rod where the sample was bonded.

A recent study utilizing a different cantilever beam tensometer [31] demonstrated the importance of also considering the mass of the cylindrical composite specimen as well as its C-factor. Because our specimens all had the same diameter, h becomes the determinant of the composite specimen mass as well as its C-factor. The measured PSD values (PSD_{meas}) for specimens with variable heights were normalized for mass to a control specimen with $h = 2.25$ mm (C-factor = 1.33) to give calculated PSD values (PSD_{calc}) using the following expression:

$$\text{PSD}_{\text{calc}} = \text{PSD}_{\text{meas}} \cdot (h_{\text{control}}/h_{\text{variable}}) \quad (7)$$

A minimum of three measurements were made for each experimental group.

1 Degree of vinyl conversion (DC). The DC attained in the TPH control composite and in the
2 experimental BT/ACP composites was measured at 23 °C by near-infrared (NIR) spectroscopy [32].
3 NIR scans (Nicolet Magna 550, Nicolet Inc., Madison, WI, USA) were taken before photo cure and 1
4 min and 2 h post-cure of composites with a thickness of approx. 3.0 mm (C-factor = 1.00 if h = 3.0
5 mm) and compared. DC corresponded to the bulk of composite and was defined as the % change in the
6 integrated peak area of the 6165 cm⁻¹ absorption band related to the first overtones of the =C-H
7 stretching vibrations of the methacrylate vinyl group (=CH₂) before and after photo-polymerization,. It
8 was calculated utilizing the following formula:

$$9 \quad DC = \{1 - [(area/thickness)_{polymer} / (area/thickness)_{monomer}]\} \times 100 \quad (8)$$

10 By measuring the thickness of monomer/polymer specimens the need to use an invariant absorption
11 band as an internal standard was circumvented.

12 Statistical data analysis. One standard deviation (SD) is identified in this paper for comparative
13 purposes as the estimated standard uncertainty of the measurements. These values should not be
14 compared with data obtained in other laboratories under different conditions. Experimental data were
15 analyzed by analysis of variance (ANOVA; $\alpha = 0.05$). Significant differences between the groups were
16 determined by all pair-wise multiple comparisons (Tukey-test).

17 **4. Conclusions**

18 The cavity design, i.e., configuration factor (C-factor) needs to be considered in minimizing the
19 polymerization stress development and, in turn, improving the quality of the interface between the
20 composite and tooth structures. However, material characteristics of the composite (filler type and
21 content, resin type, initiator system) as well as those of the dental adhesive system also can influence
22 the development of internal and interfacial stresses. Tensometry has the potential for aiding in
23 optimizing the material and processing factors that can lead to the development of polymeric materials
24 with favorable PSD values.

25 **Acknowledgements**

26 Reported work was supported by the National Institute of Dental and Craniofacial Research
27 (NIDCR)/National Institute of Standards and Technology (NIST) Interagency Agreement YI-DE-
28 7005-01 and a grant DE 13169 to the American Dental Association Foundation (ADAF). It is a part of
29 the dental research program conducted by NIST in cooperation with ADAF and was also supported by
30 both NIST and ADAF. Generous contribution of the monomers utilized in this study from Esstech,
31 Essington, PA, USA is gratefully acknowledged.

32

33

34

1 **References**

- 2 1. Bowen, R.L. Properties of Silica-reinforced polymer for Dental Restorations. *J. Am. Dent. Assoc.*
3 **1963**, *66*, 57-64.
- 4 2. Braga, R.R.; Ferracane, J.L. Alternatives in Polymerization Contraction Stress Management. *Crit.*
5 *Rev. Oral. Biol. Med.* **2004**, *15*, 176-184.
- 6 3. Bowen, R.L. Adhesive Bonding of Various Materials to Hard Tooth Tissues; VI. Forces Developing
7 in Direct-filling Materials During Hardening. *J. Amer. Dent. Assoc.* **1967**, *74(3)*, 439-445.
- 8 4. Bowen, R.L.; Nemoto, K.; Rapson, J.E. Adhesive Bonding of Various Materials to Hard Tooth
9 Tissues: Forces Developing in Composite Materials During Hardening. *J. Amer. Dent. Assoc.* **1983**,
10 *106*, 475-477.
- 11 5. Ferracane, J.L. Developing a More Complete Understanding of Stresses Produced in Dental
12 Composites During Polymerization. *Dent. Mater.* **2005**, *21*, 36-42.
- 13 6. Kinomoto, Y.; Torii, M. Photoelastic Analysis of Polymerization Contraction Stresses Between
14 Self- and Light-cured Composites. *J. Dent.* **1998**, *26*, 165-171.
- 15 7. Shono, Y.; Ogawa, T.; Terashita, M.; Carvalho, R.M.; Pashley, E.L.; Pashley, D.H. Regional
16 Measurement of Resin-dentin Bonding as an Array. *J. Dent. Res.* **1999**, *78*, 699-705.
- 17 8. Labella, R.; Lambrechts, P.; Van Meerbeek, B.; Vanherle, G. Polymerization Shrinkage and
18 Elasticity of Flowable Composites and Filled Adhesives. *Dent. Mater.* **1999**, *15*, 128-137.
- 19 9. Venhoven, B.A.M.; de Gee, A.J.; Davidson, C.L. Light Initiation of Dental Resins: Dynamics of the
20 Polymerization. *Biomaterials* **1996**, *176*, 2313-2318.
- 21 10. Feilzer, A.J.; de Gee, A.J.; Davidson, C.L. Setting Stress in Composite Resin in Relation to
22 Configuration of the Restoration. *J. Dent. Res.* **1987**, *66*, 1636-1639.
- 23 11. Hansen, E.K. Effect of Scotchbond Dependent on Cavity Cleaning, Cavity Diameter and
24 Cavosurface Angle. *Scand. J. Dent. Res.* **1984**, *92*, 141-147.
- 25 12. Giacetti, L.; Scaminaci-Russo, D.; Bambi, C.; Grandini, R. A Review of Polymerization Shrinkage
26 Stress: Current Techniques for Posterior Direct Resin Restorations. *J. Contemp. Dent. Pract.* **2006**,
27 *7(4)*, 1-13.
- 28 13. Braga, R.R.; Ferracane, J.L. Contraction Stress Related to Degree of Conversion and Reaction
29 Kinetics. *J. Dent. Res.* **2002**, *81*, 114-118.
- 30 14. Calheiros, F.C.; Braga, R.R.; Kawano, Y.; Ballester, R.Y. Relationship Between Contraction Stress
31 and Degree of Conversion in Restorative Composites. *Dent. Mater.* **2004**, *20*, 939-946.

- 1 15. Stansbury, J.W.; Trujillo-Lemon, M.; Lu, H.; Ding, X.; Lin, Y.; Ge, J. Conversion-dependent
2 Shrinkage Stress and Strain in Dental Resins and Composites. *Dent. Mater.* **2005**, *21*, 56-67.
- 3 16. Kleverlaan, C.J.; Feilzer, A.J. Polymerization Shrinkage and Contraction Stress of Dental Resin
4 Composites. *Dent. Mater.* **2005**, *21*, 1150-1157.
- 5 17. Choi, K.K.; Ruy, G.J.; Choi, S.M.; Lee, M.J.; Park, S.J.; Ferracane, J.L. Effects of Cavity
6 Configuration on Composite Restoration. *Oper. Dent.* **2004**, *29*, 462-469.
- 7 18. Uno, S.; Tanaka, T.; Inoue, S.; Sano, S. The Influence of Configuration Factors on Cavity
8 Adaptation in Compomer Restorations. *Dent. Mater. J.* **1999**, *18*, 19-31.
- 9 19. Feilzer, A.J.; de Gee, A.J.; Davidson, C.L. Quantitative Determination of Stress Reduction by Flow
10 in Composite Restorations. *Dent. Mater.* **1990**, *6*, 167-171.
- 11 20. Skrtic, D.; Antonucci, J.M.; Eanes, E.D. Amorphous Calcium Phosphate-based Bioactive
12 Polymeric Composites for Mineralized tissue Regeneration. *J. Res. Natl. Inst. Stands. Technol.* **2003**,
13 *108*, 167-182.
- 14 21. Skrtic, D.; Antonucci, J.M. Effect of Bifunctional Co-monomers on Mechanical Strength and
15 Water Sorption of Amorphous Calcium Phosphate- and Silanized Glass-filled Bis-GMA-based
16 Composites. *Biomaterials* **2003**, *24*, 2881-2888.
- 17 22. Skrtic, D.; Antonucci, J.M. Dental Composites Based on Amorphous Calcium Phosphate - Resin
18 Composition/Physicochemical Properties Study. *J. Biomat. Appl.* **2007**, *21*, 375-393.
- 19 23. Lu, H.; Stansbury, J.W.; Dickens, S.H.; Eichmiller, F.C.; Bowman, C.N. Probing the Origins and
20 Control of Shrinkage Stress in Dental Resin-composites: I. Shrinkage Stress Characterization
21 Technique. *J. Mater. Sci.: Mater. Med.* **2004**, *15*, 1097-1103.
- 22 24. Alster, D.; Feilzer, A.J.; de Gee, A.J.; Davidson C.L. Polymerization Contraction Stress in Thin
23 Resin Composite Layers as a Function of Layer Thickness. *Dent. Mater.* **1997**, *13*, 146-150.
- 24 25. Choi, K.K.; Condon, J.R.; Ferracane, J.L. The Effects of Adhesive Thickness on Polymerization
25 Contraction Stress of Composite. *J. Dent. Res.* **2000**, *79*, 812-817.
- 26 26. Watts, D. C.; Satterthwaite J. D. Axial Shrinkage Stress Depends upon Both C-factor and
27 Composite Mass. *Dent. Mater.* **2008**, *24*, 1-8.
- 28 27. Lee, S.H.; Chang, J.; Ferracane, J.L.; Lee, I.B. Influence of Instrument Compliance and Specimen
29 Thickness on the Polymerization Shrinkage Stress Measurement of Light-cured Composites. *Dent.*
30 *Mater.* **2007**, *23*, 1093-1100.
- 31 28. Munksgaard, E.C.; Hansen, E.K.; Kato, H. Wall-to-wall Polymerization Contraction of Composite
32 Resins Versus Filler Content. *Scand. J. Dent. Res.* **1987**, *95*, 526-531.

- 1 29. Feilzer, A.J.; de Gee, A.J.; Davidson, C.L. Relaxation of Polymerization Contraction Shear Stress
2 by Hygroscopic Expansion. *J. Dent. Res.* **1990**, *69*, 36-39.
- 3 30. Braem, M.; Davidson, C.L.; Vanherle, G.; Van Doren, V.; Lambrechts, P. The Relationship
4 between Testing Methodology and Elastic Behavior of Composites. *J. Dent. Res.* **1987**, *66*, 1036-1039.
- 5 31. Watts, D.C.; Marouf, A.S.; Al-Hindi, A.M. Photo-polymerization Shrinkage Stress Kinetics in
6 Resin Composites: Methods Development. *Dent. Mater.* **2003**, *19*; 1-11.
- 7 32. Stansbury, J.W.; Dickens, S.H. Determination of Double Bond Conversion in Dental Resins by
8 Near Infrared Spectroscopy. *Dent. Mater.* **2001**, *17*, 71-79.

9